CE 0123 IVD

SPIRIT HEALTHCARE

Spirit Healthcare Ltd.
Unit 3, Dunn House, 15 Warren Park Way, Enderby,
Leicester LE19 4SA, UK
Customer Support Tel : 0800 881 5423

i-SENS, Inc.
465-6 Wolgye4-dong, Nowon-gu
Seoul 139-845, Korea
www.i-sens.com

EC REP
Medical Technology Promedt
Consulting GmbH, Altenhofstrasse 80,
D-66386 St. Ingbert, Germany

ⓒ 2010 i-SENS, Inc. All Rights Reserved PGC8E3001 REV1

SPIRIT HEALTHCARE

i-sens

Owner's Booklet

CareSens™ N

Blood Glucose Monitoring System

No Coding
Easy & Accurate Testing

0.5 μl
Very Small Sample
(● : actual size shown)

5 Sec
Rapid Test Result

Welcome to the CareSens N Blood Glucose Monitoring System

Thank you for purchasing the CareSens N Blood Glucose Monitoring System. The system provides you with safe, convenient and less painful blood glucose *in vitro* (i.e., outside the body) diagnostic monitoring. You can obtain accurate results in just 5 seconds with a small (0.5 μℓ) blood sample.

Contents

Information

Important Information 6
Specifications 10
CareSens N Blood Glucose Monitoring System 11
CareSens N Blood GlucoseTest Strip 12
CareSens N Blood Glucose Meter 15
CareSens N Blood Glucose Meter Display 16

Preparation

Setting up Your System 18
- Adjusting the Date and Time 18
- Setting the Sound On/OFF 21
- Setting the Test Result Reset 22

Checking the System 24
- Control Solution Testing 26
- Comparing the Control Solution Test Results 29

Testing

Using the Lancing Device 31
- Preparing the Lancing Device 32
- Preparing the Meter and Test Strip 34
- Flagging Post-meal Test Results 34
- Applying Blood Sample 35
- Discarding Used Lancets 38

Alternative Site Testing 39
Hi and Lo Messages 43
Target Blood Glucose Ranges 44

Additional Functions

Meter Memory 45
Setting the Alarm Function 47

Maintenance

Replacing Batteries 51
Caring for Your System 53
Understanding Error and Other Messages 54
General Troubleshooting 56
Performance Characteristics 58
Warranty Information 60

Important Information: Read this First!

To receive safe and optimum system benefits, please read the entire manual contents before using the system. Please note the following instructions:

- Do not use the system for the diagnosis of diabetes without the guidance of a healthcare professional or for testing newborns.
- Use only fresh capillary whole blood samples for testing.
- Alternative site and fingertip test results may differ significantly due to rapid change in the glucose level post meal, insulin injection or exercise.

The following chart explains the symbols you'll find in the CareSens N User Manual, product packaging, and product inserts.

IVD	For in vitro diagnostic use
CE 0123	This product fulfills the requirements for Directive 98/79/EC on in vitro diagnostic medical devices.
	Cautions for safety and optimum product use
	Consult instruction for use
	Manufacturer
EC REP	Authorized representative
	Do not reuse.
LOT	Batch code
	Do not discard this product with other household-type waste
SN	Serial number
	Use by
	Temperature limitations

Important Information:

- The CareSens N blood glucose monitoring system is intended for self-testing outside the body (in vitro diagnostic use).
- The glucose in the blood sample mixes with special chemicals on the test strip where to produce a small electrical current. The CareSens N meter detects this electrical current and measures the amount of glucose in the blood sample.
- The CareSens N blood glucose meter is designed to minimize code related errors in monitoring by using the no-coding function.
- The CareSens N blood glucose meter should be used only with the strip.
- The average hematocrit(red blood cell count) range is between 30 and 50%. However, people with severe anemia, pregnant women, and newborns may have higher hematocrit and this can affect the test results.
- Very high (60% or more) or very low (20% or less) hematocrit can lead to incorrect test results.
- A glucose value of less than 3.9 mmol/L may indicate hypoglycemia and a value of more than 13.3 mmol/L may indicate hyperglycemia.

If you need assistance, please contact Spirit Healthcare or Customer Support at 0800 881 5423 for more information.

Specifications

Product specifications

Reported result range	1.1 ~ 33.3 mmol/L
Sample size	Minimum 0.5 μℓ
Test time	5 seconds
Sample type	Fresh capillary whole blood
Calibration	Plasma-equivalent
Assay method	Electrochemical
Battery life	1,000 tests
Power	Two 3.0 V lithium batteries (disposable, type CR2032)
Memory	250 test results
Size	93 X 47 X 15 (mm)
Weight	51.5 g (with batteries)

Operating ranges

Temperature	10 ~ 40˚C (50 ~ 104˚F)
Relative humidity	10 ~ 90%
Hematocrit	20 ~ 60%

CareSens N Blood Glucose Monitoring System

Components

- CareSens N Blood Glucose Meter
- CareSens N Blood Glucose Test Strip (10)
- Lancing Device
- Lancet (10)
- Owner's Booklet
- Quick Reference Guide
- Logbook
- Carrying Case
- Battery (2)

- Certain components may not be included depending on the place of purchase.
- Please contact Spirit Healthcare at 0800 881 5423 if any component is missing or damaged.
- The cable for data transmission can be ordered separately. Please contact Spirit Healthcare at 0800 881 5423.

CareSens N
Blood Glucose Test Strip

The CareSens N Blood Glucose Monitoring System measures blood glucose quickly and accurately. It automatically absorbs the small blood sample applied to the narrow edge of the strip.

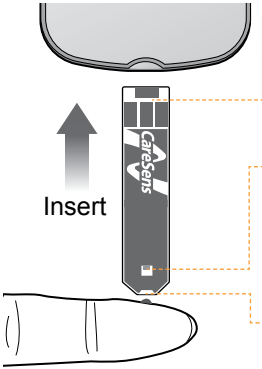

Contact bars
Gently push the test strip, with its contact bars facing up, into the test strip port of meter

Confirmation window
Check here to see whether sufficient blood sample has been applied

Edge to apply blood sample
Apply blood sample here for testing

Warning!

- The CareSens N Test Strip should be used only with fresh capillary whole blood samples.
- Do not reuse test strips.
- Do not use test strips past the expiration or discard date.
- Check the expiration date printed on the vial. When you first open a test strip vial, you must record the discard date (date opened plus six months) in the space provided on the label.
- Store test strips in a cool and dry place at a temperature of 8 ~ 30˚C (46 ~ 86˚F).
- Keep away test strips from direct sunlight or heat and do not refrigerate or freeze.
- Store test strips only in their original vial.
- Close the vial tightly after removing a test strip for testing and use the strip immediately.

- Handle test strips only with clean and dry hands.
- Do not bend, cut, or alter test strips in any way.
- For detailed storage and usage information, refer to the CareSens N Test Strip package insert.

• Caution :
Keep the meter and testing supplies away from young children.

CareSens N Blood Glucose Meter

Transmission Port
Used to transfer data from the meter to a computer with a CareSens cable

Display
Shows results, messages

↑(↓) Button
Selects or changes information

S Button
Turns the meter on/off and confirms menu selections

Test Strip Port
Insert test strip here

• Note:
The CareSens cable for data transmission to PC can be ordered separately. Please contact Spirit Healthcare at 0800 881 5423

CareSens N Blood Glucose Meter Display



alarm	appears when the time alarm has been set
mem	appears when test results stored in the memory are displayed
	appears only when the sound is set to OFF
check	appears when test results have not been saved
	test results displaying panel (Decimal point : appears when the blood glucose measuring unit is set to mmol/L)
	indicates meter battery is running low and needs to be replaced

mmol/L mg/dL	unit for measuring blood glucose
mem	appears when test results stored in the memory are displayed
	appears when the post meal alarm has been set
	appears during post-meal testing and when postmeal test results are displayed
	indicates meter is ready for the application of a drop of blood or control solution
	Month Day Hour Minute

The unit of measurement is fixed in mmol/L and it cannot be changed to mg/dL by the user.

Setting up Your System

Press and hold the **S** button for 3 seconds to switch on the meter. After all settings are finished, press and hold the **S** button for 3 seconds to turn off the meter.
Press ⬆ or ⬇ to reach the accurate value. Press and hold ⬇ to scroll faster.

Adjusting the Date and Time

Step 1 Entering the SET Mode
Press and hold the **S** button for 3 seconds to switch on the meter. After all the segments flash across the screen, the 'SET' character icon will be displayed on the screen. Press the **S** button again to enter the year setting mode.

Step 2 Setting the Year
The number that appears on the screen after the meter is turned on indicates the year of manufacture. Press and release ⬆ or ⬇ to adjust until the correct year appears. Press and hold ⬇ button to scroll through the numbers quickly. After setting the year, press the **S** button to confirm your selection and enter the month setting mode.



Step 3 Setting the Month
A number indicating the month will be blinking on the left corner of the screen. Press ⬆ or ⬇ until the correct month appears. Press the **S** button to confirm your selection and enter the date setting mode.

Step 4 Setting the Date
Press ⬆ or ⬇ until the screen displays the correct date. Press the **S** button to confirm the date and enter the time setting mode.

Step 5 Setting the Time
The meter can be set in the AM/PM 12-hour or the 24-hour clock format. Press ⬆ or ⬇ to select a format. The AM•PM icon is not displayed in the 24-hour format. After selecting the format press the **S** button to enter the hour setting mode.

Step 6 Setting the Hour
Press ⬆ or ⬇ until the correct hour appears. After the hour is set, press the **S** button to enter the minute setting mode.

Step 7 Setting the Minute
Press ⬆ or ⬇ until the correct minute appears. After setting the minute, press the **S** button to enter the sound setting mode.

Setting the Sound On/OFF

Step 8
On pressing ⬆ or ⬇, the screen will display the On or OFF. Press the **S** button to confirm the selection. The meter will beep in the following instances, if set to On.



- When the test strip is inserted in the meter
- When the blood sample is absorbed into the test strip and the test starts
- When the test result is displayed
- When you push the **S** button or ⬆ button to check the memory
- When you push the ⬆ button to set the postmeal (PP2) alarm
- When it is time for a preset blood glucose test
  If the sound is set to OFF, none of the sound functions will work.

• Note :
Only when the sound is set to OFF, 🔇 icon appears on the display.

Setting the 'Test Result Reset' (Deleting all the saved test results)

Step 9

In this mode all the test results stored in the meter can be deleted. Please note that if you select YES, all the stored test results will be deleted and can not be restored. After the beeper mode is set, press the **S** button to enter the 'Test Result Reset' mode. The 'dEL' character will blink on the screen.

Press ⬆ or ⬇ to alternate between 'YES' or 'no'. To delete all the stored test results press the **S** button while the screen displays 'YES'. Then, all the test results stored in the meter will be deleted and the screen will be similar to the picture on the right. If you do not want to delete the results press the **S** button while the screen displays 'no'. Then, the screen will return to step 2. See page 18.

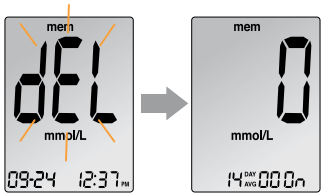

• Note :

At any stage, if the **S** button is pressed for 3 seconds, Time and Date setting mode will finish and the meter will be turned off. Press and hold ⬇ to scroll through numbers quickly.

Checking the System

You may check your meter and test strips using the CareSens Control Solution.
The CareSens Control Solution contains a known amount of glucose and is used to check that the meter and the test strips are working properly.
The test strip vials have CareSens Control Solution ranges printed on their labels.
Compare the result displayed on the meter to the CareSens Control Solution range printed on the test strip vial.
Before using a new meter or a new vial of test strips, you may conduct a control solution test following the procedure on page 26.



• Notes :
- Use only the CareSens Control Solution.
- Check the expiration dates printed on the vial. When you first open a control solution vial, record the discard date (date opened plus three months) in the space provided on the label.
- Make sure your meter, test strips, and control solution are at room temperature before testing. Control Solution tests must be done at room temperature (20 ~ 25˚C, 68 ~ 77˚F).
- Before using the control solution, shake the vial, discard the first few drops and wipe the tip clean.
- Close the control solution vial tightly and store at a temperature of 8 ~ 30˚C (46 ~ 86˚F).

• You may do a control solution test:
- When using the meter for the first time
- Whenever you open a new vial of test strips
- If the meter or test strips do not function properly
- If your symptoms are inconsistent with the blood glucose test results and you feel that the meter or test strips are not working properly
- If you drop or damage the meter

Step 3
A test result will appear after the meter counts down from 5 to 1. After your control solution result appears on the display, press ⬇ for 3 seconds till the 'check' icon appears on the display. When the 'check' icon is displayed, the result is not stored in the meter's memory and is not included in the 14-day averages.

Step 4
Compare the result displayed on the meter to the range printed on the test strip vial. The result should fall within that range. Used strips should be discarded safely in disposable containers.

• Caution :
- If the results you get are not within this range, the meter and test strip may not work properly. Then, stop using the meter and contact the Spirit Healthcare at 0800 881 5423.
- The range printed on the test strip vial is for the CareSens Control Solution only. It does not have any connection to your blood glucose level.

Comparing the Control Solution Test Results

Repeat the control test if the test result falls outside the range printed on label of the test strip vial. Out of range results may occur due to the following factors:

- When the control solution vial was not shaken well,
- When the control solution is past its expiration date or is contaminated,
- When the meter, the strip or the control solution were exposed to high or low temperatures,

- When the first few drops of the control solution were not discarded or the tip of the vial was not wiped clean,
- When the test strip is past its expiration date,
- When the meter is not functioning properly.

• Note :
The CareSens Control Solution can be purchased separately. Please Contact Spirit Healthcare at 0800 881 5423.

Using the Lancing Device

You will need a lancing device in order to collect a blood sample. You may use the lancing device contained in the CareSens N Blood Glucose Monitoring System or any other medically approved lancing device.

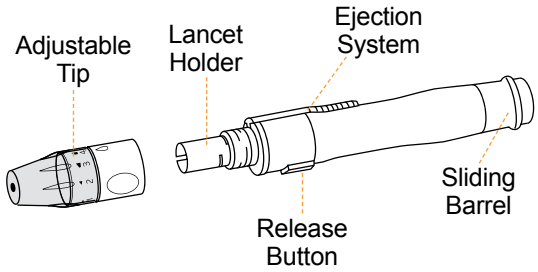

- The lancing device should be used by one individual.
- Use a soft cloth or tissue to wipe the lancing device. If necessary, a small amount of alcohol on a soft cloth or tissue may be used.

• Caution :

To avoid infection when drawing a sample, use a lancet only onetime, and:

- Do not use a lancet that has been used by others.
- Always use a new sterile lancet.
- Keep the lancing device clean.

• Note :

Repeated puncturing at the same sample site may cause pain or skin calluses. Choose a different site each time you test.

Preparing the Lancing Device

Step 1
Wash hands and fingertip sample site with soap and warm water. Rinse and dry thoroughly.



Step 2
Unscrew lancing device tip thoroughly.



Step 3
Firmly insert new lancet into lancet holder. Hold lancet firmly. Gently twist to pull off protective disk. Save disk to recap lancet after use. Replace lancing device tip.



Step 4
Select a desired depth of one-to-five (1-5) on lancing device's adjustable tip. Rotate ring to align desired number with arrow. A beginning setting of three (3) is recommended.



Step 5
To cock the lancing device, hold the tip in one hand. Pull the sliding barrel on with the other hand. The lancing device is cocked when you feel a click.



• Note :
The skin depth to retrieve samples will vary for various people at different sample sites. The lance's adjustable tip allows the best depth of skin penetration for an adequate sample size. A beginning setting of three (3) is recommended.

Preparing the Meter and Test Strip

Step 6



Insert a test strip with the contact bars facing upwards into the meter's test strip port. Push the strip in gently until the meter beeps. Be careful not to bend the test strip.
The ▬◂ symbol will appear on the screen.

Flagging Post-meal Test Results

The meter allows you to flag a result of an post-meal test with (🍴) icon. The post-meal test flag (🍴) can be attached just before applying the blood sample. Once you attach the post-meal flag (🍴) to the test results, it cannot be deleted.

Step 7



If you want to attach an post-meal flag (🍴) to a test result, press and hold ▼ for 3 seconds after inserting the test strip.
The post-meal flag (🍴) and the ▬◂ symbol will appear on the screen. The test result will also be displayed with the post-meal flag (🍴).
If you do not want to save the result as an postmeal test, move on to the step 8 after the step 6.

Applying Blood Sample

Step 8



Obtain a blood sample using the lancing device. Place the device against the pad of the finger. The best puncture sites are on the middle or ring fingers. Press the release button. Remove the device from the finger. Wait a few seconds for a blood drop to form.
A minimum volume of 0.5 microliter is needed to fill the confirmation window.
(actual size of 0.5 μℓ : ●)

Step 9

After the symbol appears on the screen, apply the blood sample to the narrow end of the test strip till the meter beeps. If the confirmation window is not filled before the meter finishes counting down then discard the test strip and insert a new one. If confirmation window is not filled in time because of abnormal viscosity or insufficient volume, Er4 message will appear.

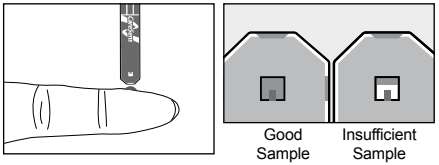

• Note :

The meter may switch off if the blood sample is not applied within 2 minutes of the icon appearing on the screen. If the meter turns off, remove the strip and reinsert after switching on the meter.

Step 10

The test result will appear after the meter counts down from 5 to 1. The result will be automatically stored in the meter's memory. If the test strip is removed after the test result is displayed, the meter will automatically switch off after 3 seconds.

Discard used test strips safely in disposable containers.

Discarding Used Lancets

Step 1
Unscrew general lancing device tip.



Step 2
Place protective cover on lancet. Pull out the sliding barrel and simultaneously push the lancet ejector forward with the thumb to dispose of used lancet in a proper biohazard container.



• Caution :
The lancet is for single use only. Never share or reuse a lancet.
Always dispose of lancets properly.

Alternative Site Testing

What is AST(Alternative Site Testing)?

Usually, when someone tests their glucose, they take the blood sample from the tip of the finger. However, since there are many nerve endings distributed there, it is quite painful. When doing a glucose test, using different parts of the body such as the arms, palms, thighs, and calves can reduce the pain during testing. This method of testing with different parts of the body is called Alternative Site Testing. While AST may reduce the pain during testing, it may not be simple for everyone and the following precautions should be observed during testing.

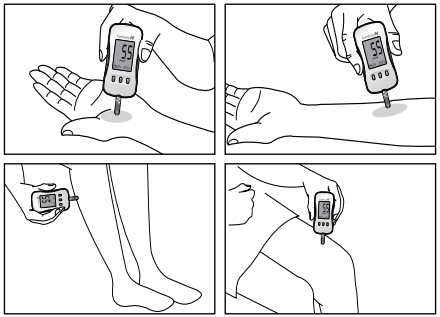

Alternative Site for Testing

Things to know when using AST

Please understand the following things before testing outside of the fingertip (arms, thighs, calves).
The capillary blood of the fingertip shows the change in glucose more rapidly than AST. Therefore, the test results from the fingertip test and AST may differ. This is because things such as lifestyle and ingested food have an effect on glucose levels.

Acceptable situations for AST

- Fasting period
- Before a meal
- Before sleeping

Situations requiring fingertip test

- When the glucose levels are rapidly increasing during the two hours after a meal or exercise
- When sick or when glucose levels seem quite lower than test value
- When hypoglycemia is not well recognized
- When insulin has the biggest effect
- 2 hours after an insulin injection

AST Precautions

- Do not ignore the symptoms of hyperglycemia or hypoglycemia.
- When the results of the test do not reflect one's opinion, retest using the fingertip test. If the test results do not reflect one's opinion, please consult a doctor.
- Do not rely on the AST results for changing one's treatment method.
- The amount glucose in alternative sites differs from person to person.
- Before using AST, please consult your regular physician.

• Note :
Results from alternative site and fingertip samples may appear differently as there is a time lag for the glucose levels to reach the same value. Use a fingertip for drawing if you suffer from hypoglycemia or have experienced hypoglycemic shock or symptoms.

• Note :
If the sample drop of blood runs or spreads due to contact with hair or with a line in you palm, do not use that sample.
Try puncturing again in a smoother area.

HI and Lo Messages

HI Message

The meter displays results between 1.1 ~ 33.3 mmol/L. The HI icon appears when the blood glucose level is more than 33.3 mmol/L and indicates hyperglycemia.
If the HI icon is displayed again on retesting, please contact your healthcare professional immediately.

Lo Message

The Lo icon appears when the result is less than 1.1 mmol/L and indicates hypoglycemia. If the Lo icon is displayed again on retesting, please contact your healthcare professional immediately.

• Note :
Please contact Spirit Healthcare Customer Support at 0800 881 5423 if such messages are displayed even though you do not have hyperglycemia or hypoglycemia.

Target Blood Glucose Ranges

Reminders Time of day	Your target ranges from your healthcare expert
Before breakfast	
Before lunch or dinner	
1 hour after meals	
2 hours after meals	
Between 2 a.m. and 4 a.m.	

Source : Diagnosis of Diabetes, NIH Publication No. 05-4642, January 2005

Meter Memory

The CareSens N meter can save up to 250 glucose test results with time and date. If the memory is full, the oldest test result will be deleted and the latest test result will be stored.
The CareSens N meter calculates and displays the averages of total test results, pre-meal test results, and post-meal test ( ) results from the last 14 days.

Viewing Test Results Stored in the Meter's Memory

Step 1
Press the ⬆ or **S** button to turn the meter on. The current date and time will be displayed on the bottom of the screen for 2 seconds, followed by the average value and the number of the test results saved within the last 14 days.

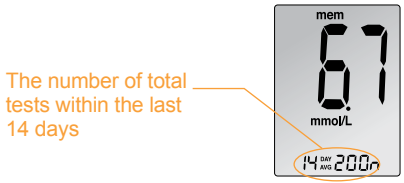

Step 2
Press ⬇ to view the average value and the number of tests performed before eating a meal for the last 14 days. On pressing ⬇ again, the average value and the number of tests performed post meals for the same period will appear on the screen.

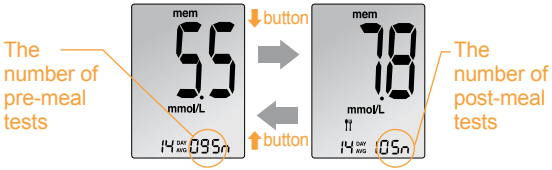

Step 3
Use the ⬇ button to scroll through the test results, starting from the most recent and ending with the oldest. Press ⬆ to return to the result seen previously. After checking the stored test result, press the **S** button to turn off the meter.

• Note :
On pressing ⬇, the latest test result saved in the meter's memory will be displayed on the screen along with the date and time. Press and hold ⬇ to scroll through the test results.

Setting the Alarm Function

Four types of alarms can be set in the CareSens N meter: one post-meal alarm (PP2 alarm) and three time set alarms (alarm1 ~ 3). The PP2 alarm goes off 2 hours after setting the alarm.
The alarms ring for 15 seconds and can be silenced by pressing ⬆, ⬇ or the S button or by inserting a test strip.

Setting the post-meal alarm (PP2 alarm)

Step 1 Setting the PP2 alarm On
Without inserting a test strip, press and hold ⬆ for 3 seconds to set the post-meal alarm. The 'PP2' character, the bell (🔔) icon and then the 'On' character will be displayed. The screen will then automatically change to the memory check mode. At this time, the bell (🔔) icon, indicating that the PP2 alarm has been set, will be displayed on the screen.



Step 2 Setting the PP2 alarm OFF

To turn off the PP2 alarm, press and hold ↑ for 3 seconds. The 'PP2'character, the bell (🔔) icon and then the 'OFF' character will appear on the screen. Then the screen will change automatically to the memory check mode without the bell (🔔) icon being displayed.

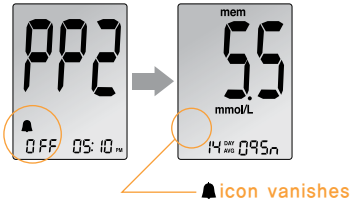

Setting the Time Alarms (alarm1 ~ 3)

Step 1

Without inserting a test strip, press ↑ and the S button simultaneously for 3 seconds to enter the time alarm mode. The 'alarm1' will be displayed while the 'OFF' character blinks on the screen.

Step 2

On pressing ↓, the 'alarm1' is set and the 'On' character is displayed on the screen. Press ↓ again to cancel the 'alarm1'. The 'OFF' icon will blink on the screen .

Step 3

Press ↑ to adjust the time of the 'alarm1'. A number representing the time will blink on the screen. Press ↓ to set the time. Press ↑ to end.

Step 4
On pressing ⬆, the number indicating the minute will start blinking. Press ⬇ to set the accurate minute.

Step 5
Press the **S** button to finish and to enter the 'alarm 2' mode. Repeat steps 2 to 5 to set the remaining time alarms (alarm 2 ~ 3).

Step 6
Press the **S** button for 3 seconds to finish and turn the meter off.

Replacing Batteries

The CareSens N meter comes with two 3.0 V lithium batteries. When the ▭ icon appears on the display for the first time, the battery should be replaced as soon as possible. The test results might not be saved if the battery runs out.

Step 1
Make sure the meter is turned off. Push the cover in the direction of the arrow to open the battery compartment.



Step 2
Remove the old battery by lifting the battery with the index finger and pulling out the battery with your thumb and index fingers as shown in the figure on the right one by one. Insert two new batteries with the + side facing up and make sure the battery is inserted firmly.



Step 3
Place the cover on the battery compartment.
Push down until you hear the tab click into place.



• Note :
Removing the meter batteries will not affect your stored result.
However, you may need to reset your meter settings. See pages 18 ~ 23.

Caring for Your System

Use a soft cloth or tissue to wipe the meter exterior. If necessary, the soft cloth or tissue might be dipped in a small amount of alcohol.
Do not use organic solvents such as benzene, or acetone, or household and industrial cleaners that may cause irreparable damage to the meter.
Store all the meter components in the portable case to prevent loss.

• Caution

- Do not expose the meter to direct sunlight or heat for an extended period of time.
- Prevent the entry of dirt, dust, blood, or water at the meter's test strip port.
- Do not drop the meter or submit it to strong shocks.
- Do not try to fix or alter the meter in any way.
- Keep the meter in a cool and airy place.
- Keep the meter away from strong electromagnetic fields such as cell phones and microwave ovens.
- CareSens N meter should be used only with CareSens N strips.

Understanding Error and Other Messages

	A used test strip was inserted. • Repeat the test with a new test strip.
	The blood or control solution sample was applied before the icon appeared. • Repeat the test with a new test strip and wait until the icon appears before applying the blood sample.
	The temperature during the test was above or below the operating range. • Move to an area where the temperature is within the operating range (10 ~ 40˚C/50 ~ 104˚F) and repeat the test after 30 minutes.
	The blood sample has abnormally high viscosity or insufficient volume. • Repeat the test after inserting a new test strip.
	Test strip was not inserted properly. • Insert a test strip with the contacting bars facing upwards and push in gently until the meter beeps.
	There is a problem with the meter. • Do not use the meter. Contact Spirit Healthcare Customer Support at 0800 881 5423.

• Note :
If the error messages persist, contact Spirit Healthcare Customer Support at 0800 881 5423.

General Troubleshooting

Problem	Troubleshooting
The display is blank even after inserting a test strip.	• Check whether the test strip is inserted with the contact bars facing up. Check if the strip has been inserted completely till the end. • Check whether the batteries are inserted with the '+' side facing up. • Replace the batteries.
The test does not start even after applying the blood sample on the strip.	• Check if the confirmation window is filled adequately. • Repeat the test after inserting a new test strip.

Problem	Troubleshooting
The test result doesn't match your expectation.	• Repeat the test after inserting a new test strip. • Check the validity period of the test strip. • Check if the strip has passed the discard date (date of opening the test strip vial plus 6 months). • Check the meter.

• Note :
If the problem is not resolved, please contact Spirit Healthcare Customer Support at 0800 881 5423.

Performance Characteristics

The performance of CareSens N Blood Glucose Monitoring System Strips has been evaluated in laboratory and in clinical tests.

Accuracy: The accuracy of the CareSens N BGM System (Model GM505NA, GM505NB, GM505NC) was assessed by comparing blood glucose results obtained by patients with those obtained using a YSI Model 2300 Glucose Analyzer, a laboratory instrument . The following results were obtained by 110 diabetic patients at clinic centers.

Slope	0.961
Y-intercept	0.194 mmol/L
Correlation coefficient(r)	0.995
Number of sample	110
Range tested	1.7 ~ 26.9 mmol/L

Accuracy results for glucose concentration<4.2mmol/L

Within ± 0.28 mmol/L	13/17 (76%)
Within ± 0.56 mmol/L	16/17 (94%)
Within ± 0.83 mmol/L	17/17 (100%)

Accuracy results for glucose concentration≥4.2mmol/L

Within ± 5%	45/93 (48%)
Within ± 10%	88/93 (96%)
Within ± 15%	93/93 (100%)
Within ± 20%	93/93 (100%)

Precision: Precision studies were performed in a laboratory using the CareSens N BGM System.

Within Run Precision		
Blood average	2.1 mmol/L	SD = 0.11 mmol/L
Blood average	4.8 mmol/L	CV = 3.7%
Blood average	6.9 mmol/L	CV = 4.1%
Blood average	10.5 mmol/L	CV = 2.6%
Blood average	18.6 mmol/L	CV = 2.8%

Total Precision		
Control average	2.4 mmol/L	SD = 0.11 mmol/L
Control average	6.3 mmol/L	CV = 3.3%
Control average	21.2 mmol/L	CV = 4.2%

This study shows that there could be variation of up to 4.2%

SPIRIT HEALTHCARE

Warranty Information

Manufacturer's Warranty

i-SENS, Inc. warrants that the Meter shall be free of defects in material and workmanship in normal use for a period of five(5) years. The meter must have been subjected to normal use.
The warranty does not cover improper handling, tampering, use, or service of the meter. Any claim must be made within the warranty period.

The i-SENS company will, at its discretion, repair or replace a defective meter or meter part that is covered by this warranty. As a matter of warranty policy, i-SENS will not reimburse the consumer's purchase price.

Obtaining Warranty Service

To obtain warranty service, you must return the defective meter or meter part to Spirit Heathcare. Please contact Customer Support on 0800 881 5423 for further information.